

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problems Mailbox.**

THIS PAGE BLANK (USPTO)



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification⁶:

A61M 25/00

A1

(11) International Publication Number:

WO 99/26691

(43) International Publication Date:

3 June 1999 (03.06.99)

(21) International Application Number: PCT/US98/24927

(22) International Filing Date: 25 November 1998 (25.11.98)

(30) Priority Data:

08/977,815 25 November 1997 (25.11.97) US

(71) Applicant: ADVANCED CARDIOVASCULAR SYSTEMS, INC. [US/US]; 3200 Lakeside Drive, P.O. Box 58167, Santa Clara, CA 95052-8167 (US).


(72) Inventors: LEE, Jeong, Soo; 23637 E. Goldrush Drive, Diamond Bar, CA 91765 (US). WANTINK, Kenneth, L.; 33583 Vino Way, Temecula, CA 92591 (US). TANNIER, Alan, A.; 26531 Ynez Road, Temecula, CA 92591 (US). TIERNAN, Stephen, J.; 131 Santa Rita Avenue, Palo Alto, CA 94301 (US).

(74) Agents: LYNCH, Edward, J.; Heller, Ehrman, White & McAuliffe, 525 University Avenue, Palo Alto, CA 94301-1900 (US) et al.

(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

Published*With international search report.**Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.*

(54) Title: CATHETER MEMBER WITH BONDABLE LAYER

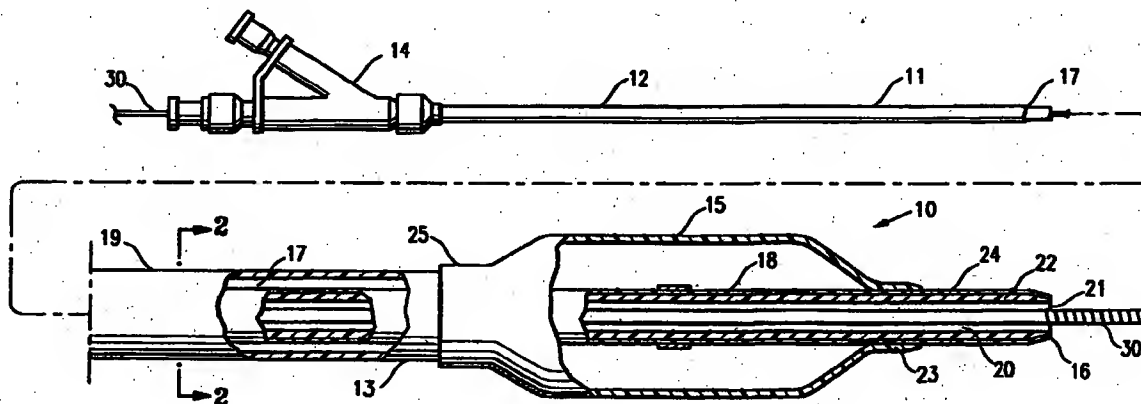

(57) Abstract

The invention is directed to a catheter formed at least in part of a multilayered member having a first layer which is fusion bondable to another catheter component such as the skirt of an inflatable balloon and a second layer which is adjacent the first layer having a melting point greater than the first layer so that the multilayered member of the catheter is not deformed when the other catheter component is fusion bonded to the first layer of the multilayered member. The second layer is preferably lubricious in nature. In one embodiment of the invention, the multilayered member is a tubular element with the lubricious second layer defining an inner lumen extending within the tubular element. The outer layer of the tubular member may extend beyond the distal end of the inner layer and form a non-traumatic distal tip. Alternatively, a flexible non-traumatic distal tip may be fusion bonded to at least the outer layer of the multilayered tubular member.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

CATHETER MEMBER WITH BONDABLE LAYER**BACKGROUND OF THE INVENTION**

This invention generally relates to intravascular catheters, particularly catheters for use in percutaneous transluminal coronary angioplasty (PCTA) or for the delivery of stents.

In a typical PTCA procedure a dilatation balloon catheter is advanced over a guidewire to a desired location within the patient's coronary anatomy where the balloon of the dilatation catheter is properly positioned within the stenosis to be dilated. The balloon is then inflated with radiopaque liquid at relatively high pressures (generally 4-12 atmospheres) to dilate the stenosed region of the diseased artery. One or more inflations may be needed to effectively dilate the stenosis. The catheter may then be withdrawn from the stenosis or advanced further into the patient's coronary anatomy to dilate additional stenoses.

In addition to the dilation of stenoses, balloon catheters similar to those described above are used to deploy stents within a patient's body lumen after a dilatation has been completed or simultaneously with the dilatation in order to maintain lumen patency. In this case an expandable stent is disposed about the exterior of the balloon on the distal extremity of the catheter and the catheter is then advanced within the patient's body lumen until the stent mounted on the exterior of the balloon is at the location in which the stent is to be deployed, e.g. usually at the stenotic site of a previous dilatation. The balloon is inflated so as to expand the stent against the wall defining the body lumen and then the balloon is deflated and the catheter withdrawn from the patient's body lumen.

Advances in the development of balloon catheters for both dilatation and stent deployment have made the selection of materials difficult because of conflicting requirements. For example, higher dilation pressures has made the sealed bonding of the balloon the catheter shaft a greater requirement, but the materials from which the high pressure balloons are made, e.g. polyethylene terephthalate, polyamide (e.g. nylon) and the like, have limited the materials to which the balloon can be bonded, and thus, the materials from which the catheter shaft can be made, particularly the distal extremity of the catheter shaft where the balloon is located.

If the distal tip of an intravascular catheter is to have non-traumatic characteristics to minimize damage when passing through a body lumen, additional material limitations come into play because typical non-traumatic tips are formed from short tubular members made of relatively soft polymeric material which are
5 secured by adhesive or fusion bonding to the distal tip of the tubular distal extremity of the catheter.

Other complicating factors in the selection of materials for intraluminal catheters is the usual requirement that the proximal shaft be much longer and much less flexible than the distal shaft section so that the proximal shaft section provides
10 the push to the catheter and so that the more flexible distal shaft section can be readily advanced through tortuous anatomy.

The difficulties in material selection and the more complicated construction of the more recently developed catheters make their manufacture more difficult and more expensive. What has been needed is a catheter structure which simplifies the
15 material selection and reduces the cost of manufacture. The present invention satisfies these and other needs.

SUMMARY OF THE INVENTION

This invention is directed to an improved multilayer member for an intraluminal catheter which can be readily bonded to other catheter parts.

20 The multilayer member of the invention has a first layer which is fusion bondable to another catheter component and an adjacent second layer which has greater lubricity than the first layer. The first layer preferably has a melting point which is lower than the melting point of the adjacent second layer so that when the first layer is fusion bonded to another catheter component, the adjacent layer of the
25 multilayer member is not deformed or otherwise misshapen by the heat from a bonding procedure. In a presently preferred embodiment of the invention, the multilayered member is in a tubular form with the second layer on the inside of the tubular member defining an inner lumen extending through the tubular member. The first layer which has a melting point lower than that of the second layer forms at least
30 in part the outer layer of the tubular member.

In one aspect of the invention, the catheter has an elongated shaft with a proximal end, a distal end, a port in the distal end and a guidewire lumen extending

through at least the distal portion of the catheter to and in fluid communication with the port in the distal end of the catheter shaft. In accordance with this aspect, the elongated shaft of the catheter has a multilayer tubular member with a first or outer layer which is fusion bondable to another catheter component and a second or inner layer which has lubricious properties. A high strength outer layer may be bonded to at least part of the first layer to provide additional strength and pushability. The first layer should have a melting point which is at least 20° C., preferably at least 30° C. lower than the melting point of an adjacent polymeric layer, so that the adjacent layer is not distorted by the heat from the fusion bonding procedure.

The material from which the first layer of the multilayered member, which has a lower melting point than the adjacent second layer, is selected so as to be compatible with the polymeric material of the catheter component to which it is to be secured. A presently preferred lower melting point polymeric material is a polyolefin based copolymer with not more than 35% (by weight) reactive monomer forming the copolymer. A suitable polyolefin material is copolymerized with one or more monomers selected from the group consisting of carboxylic acid or acrylic acid or anhydride thereof and preferably is unsaturated. A presently preferred polyolefinic material is a polyethylene based adhesive polymer such as ethylene-acrylic acid copolymer which is sold commercially as PRIMACOR by Dow Chemical Co. or as ESCOR by EXXON or as PLEXAR by Quantum Chemical Corp. Other suitable materials include polymers which have been modified by reactive extrusion having a durometer range of about Shore A 80 to about Shore D 80, preferably about Shore A 90 to about Shore D 70.

The second or inner layer of the multilayer member having lubricious properties should have a coefficient of friction (both static and dynamic) of less than 0.35 and preferably less than 0.30. Suitable polymeric materials having the aforesaid coefficient of friction include polyethylene, polytetrafluoroethylene and other fluoropolymers.

As previously mentioned a third layer may be provided on the side of the first layer opposite side in contact with the second layer and may be formed of various polymeric materials to provide a catheter shaft with additional push and to prevent collapse or kinking of the tubular member in manufacturing or use. Suitable

polymeric materials for the third layer include high density polyethylene, polyethylene terephthalate (PET), polyamide, a thermoplastic polyurethane, polyetheretherketone (PEEK) and the like.

5 All or most of the layers of the multilayered tubular member are preferably selected or modified so that they can be melt processed, e.g. coextruded, simultaneously or sequentially, and as a result the polymeric materials of the various layers should be compatible in this regard or made compatible by appropriate additives to the polymers.

10 In one presently preferred embodiment of the invention, the catheter is a dilatation catheter for angioplasty or stent delivery having a balloon on a distal shaft section with a multilayered inner tubular member which extends through and distal to the balloon and which defines at least in part a guidewire lumen extending to and in fluid communication with a port in the distal end of the catheter. In this instance, the multilayered inner tubular member has a bondable outer layer and the polymeric
15 material thereof is selected to facilitate the fusion bonding of the distal skirt of the balloon to the outer layer of the inner tubular member. The multilayered inner tubular member also has an inner layer having lubricious properties which defines at least part of the guidewire lumen.

20 Another embodiment of the invention is directed to an intraluminal catheter wherein the multilayered tubular member forms at least part of the shaft of the intraluminal catheter and the low melting point material of the outer bonding layer of the multilayered tubular member extends beyond an adjacent layer to form a non-traumatic distal tip on the catheter shaft.

25 In yet another aspect of the invention, the catheter is provided with a non-traumatic distal tip which is fusion bonded to at least the bondable layer on the multilayered tubular member. While a fusion bond somewhat limits the selection of material for the bondable layer, the preferred material discussed above, namely the polyethylene based adhesive such as PRIMACOR, ENCOR or PLEXAR facilitates fusion bonding to a wide variety of materials including polyethylene, PET, polyamide,
30 polyurethane, PVC and copolymers such as PEBAX® and HYTREL® and the like.

In most instances the wall thickness of the fusion bondable layer of the multilayered tubular member should be less than half the wall thickness of the

tubular member, preferably less than 40% of the total thickness of the member. The inner and outer dimensions of the tubular member generally follow the dimensions of other tubular members from which intravascular catheters are made.

5 The present invention provides an improved multilayered member which greatly facilitates bonding of one catheter component to another catheter component, particularly bonding the skirt of dilatation balloon to the inner tubular member of the catheter.

10 These and other advantages of the invention will become more apparent from the following detailed description of the invention when taken in conjunction with the accompanying exemplary drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is an elevational schematic view, partially in section, of a dilatation catheter embodying features of the invention.

15 Fig. 2 is a transverse cross-sectional view of the catheter shown in Fig. 1 taken along the lines 2-2.

Fig. 3 is an elevational view, partially in section, of an alternative embodiment of the invention wherein a dilatation catheter has an outer tubular member with multiple layers.

20 Fig. 4 is a transverse cross-sectional view similar to the view shown in Fig. 2 of an alternative embodiment with the inner tubular member having three layers of polymeric material.

Fig. 5 is an elevational schematic view, partially in section, of the distal portion of another alternative embodiment of the invention wherein the outer layer of a tubular member of the catheter forms a non-traumatic distal tip on the catheter.

25 Fig. 6 is an elevational view, partially in section, of another embodiment of the invention, illustrating a non-traumatic distal tip bonded to the distal end of a multilayered inner tubular member.

30 Fig. 7 is an elevational view, partially in section, of another embodiment of the invention, illustrating a non-traumatic distal tip bonded to the distal end of a multilayered inner tubular member where the non-traumatic distal tip is a multilayered tubular member.

DETAILED DESCRIPTION OF THE INVENTION

Reference is made to Figs. 1-2 which illustrate a balloon dilatation catheter 10 embodying features of the invention. Catheter 10 has an elongated shaft 11 with proximal and distal shaft sections 12 and 13, an adapter 14 on the proximal end of the shaft and a dilatation balloon 15 on the distal shaft section spaced proximal to the distal end 16. An inflation lumen 17 extends between the proximal end of shaft 11 and a location spaced proximal to the distal end 16 and is in fluid communication with the interior of the dilatation balloon 15. The catheter shaft 11 is provided with a multilayered first inner tubular member 18 and an outer tubular member or jacket 19 of suitable polymeric material or materials. A guidewire receiving lumen 20 extends through the proximal and distal shaft sections 12 and 13 to the port 21 in the distal end of the shaft 11. In the distal shaft section 13, the guidewire receiving lumen 20 is defined at least in part by the inner layer 22 of the first inner tubular member 18.

The balloon 15 has a distal skirt 23 which is secured by fusion bonding to lower melting point polymeric material of the outer layer 24 of the multilayered first inner tubular member 18 and a proximal skirt 25 which is secured by suitable means to the distal end of the outer tubular member 19.

The multilayered tubular members of the invention may have more than two layers in other configurations. For example, as shown in Fig. 4, a high strength outer layer 29 may be provided on the exterior of low melting point bonding layer 24. While not shown in the drawings the high strength outer layer 29 may be removed from the distal portion of the inner tubular member 18 to expose the low melting point bonding layer 24. In this manner the outer layer 29 can provide strength and torqueability to the inner member 18 but the exposed part of the bonding layer 22 would still be available for bonding to the distal skirt 23 of the balloon 15. As shown in Figs. 1-4 a guidewire 30 is slidably disposed within the inner lumen 20 of the inner tubular member 18.

The multilayered tubular members described above may be readily formed by coextruding at least two of the layers thereof, and preferably all of the layers. The lubricious layer may be a hydrophilic or otherwise lubricious polymeric material which may be a homopolymer, a copolymer or a blend of polymeric materials having at least one component which develops a lubricious surface.

A further modification of the present invention is illustrated in Fig. 5 which depicts the distal extremity of an intravascular catheter 40 formed of a multilayered tubular member 41 wherein the outer layer 42 extends beyond the distal end of the inner layer 43 and is heat shaped so as to form a non-traumatic distal tip 44. A presently preferred method of forming the non-traumatic distal tip 44 is to heat shape the distal portion of the outer layer 42 which extends distally beyond the distal end of the inner layer 43 against the exterior of a mandrel (not shown) disposed within the guidewire lumen 45 and an exterior shaping member which heat forms the exterior of the distal tip 44.

Fig. 6 shows a distal extremity of an intravascular catheter 50 formed in part from a multilayered tubular member 51 having an outer layer 52 formed of bondable polymeric material as previously described, an inner layer 53 and a flexible distal tip 54 which is fusion bonded at least to the distal end or the exterior of the outer layer.

An alternative embodiment of an intravascular catheter 60, as shown in Fig. 7, has a multilayered tubular member 61 with an outer layer 62 formed of the lower melting point polymeric material as previously described, an inner lubricious layer 63 and a flexible distal tip 64 bonded to the end or exterior or both of the outer layer 62. The embodiment of Fig. 7 differs from that shown in Fig. 6 by having a multilayered distal tip 64 with an outer layer 65 and an inner layer 66. Preferably, the inner layer 66 is formed of a low melting point polymeric material the same as or compatible with the outer layer 62 to facilitate fusion bonding of the distal tip 64 to the exterior of the tubular member 61.

The thickness of the bonding layer generally will depend upon the material from which the layer is formed and the stresses to which the bonding layer will be exposed to in use. The dimensions of the various catheter components of the invention may generally follow the dimensions of similar components utilized in commercially available catheters. For example, for angioplasty catheters and stent delivery catheters the guidewire lumen should accommodate the guidewire having diameters of about 0.010 to 0.035 inch (0.25-0.89 mm), typically about 0.012 to about 0.018 inch (0.30-0.46 mm) so the guidewire receiving lumen should range from about 0.014 to about 0.040 inch (0.36-1.0 mm), preferably about 0.016 to about 0.023 inch (0.38-0.58 mm). If the catheter is to have perfusion capabilities, the

number, size and distribution of perfusion holes in the catheter wall (not shown) is controlled to provide a perfusion flow rate of about 20-60 cc/min, preferably about 30-45 cc/min. The inflated balloon diameters may range from about 1 to about 5, typically about 2 to about 4 mm. Balloon lengths may range from about 10-50 mm, typically about 20-40 mm. The distal shaft section proximal to the balloon may range from about 0.03 to about 0.06 inch (0.76-1.52 mm), typically about 0.035 to about 0.05 inch (0.89-1.27 mm). Balloon burst pressures should be about 10 to about 20 atmospheres (147-294 psi), preferably about 12 to about 15 atmospheres (176-221 psi). To the extent not described herein dimensions and materials described in the references incorporated herein and dimensions and materials used in commercially available dilatation and stent delivery catheters may be employed with the catheters of the present inventions.

The catheter of the invention may be of a rapid exchange type catheter such as described in U.S. Patent No. 5,040,548 (Yock), U.S. Patent No. 4,748,982 (Horzewski *et al.*), U.S. Patent No. 5,496,275 (Sirhan *et al.*) and U.S. application Serial No. 08/484,267, filed on June 7, 1995, which have been incorporated herein. In these catheters the guidewire lumen extends from a distal port in the distal end of the catheter shaft to a proximal port spaced proximally about 7 to about 45 cm, preferably about 15 to about 35 cm, from the distal end of the catheter shaft.

Although individual features of embodiments of the invention may be shown in some of the drawings and not in others, those skilled in the art will recognize that individual features of one embodiment of the invention can be combined with any or all the features of another embodiment. Moreover, various modifications can be made to the present invention without departing from the scope thereof.

WHAT IS CLAIMED IS:

1. An intraluminal catheter comprising:
 - a) an elongated shaft having proximal and distal ends, a port in the distal end and a guidewire lumen extending therein to and in fluid communication with the port in the distal end;
 - b) a multilayered tubular member defining at least in part the guidewire lumen, having an inner layer formed of a lubricious polymeric material and a readily bondable outer layer formed of a polymeric material having a melting point lower than that of the inner layer; and
 - c) a catheter part fusion bonded to the outer layer of the multilayered tubular layer.
2. The catheter of claim 1 wherein the catheter part is a distal skirt of a balloon.
3. The catheter of claim 1 wherein the inner layer of the multilayered tubular member has a static coefficient of friction of less than about 0.35.
4. The catheter of claim 1 wherein the inner layer of the multilayered tubular member has a static coefficient of friction of less than about 0.30.
5. The catheter of claim 1 wherein the outer layer is a polyolefin adhesive polymer.
6. The catheter of claim 5 wherein the polyolefin has up to 30% by weight of a copolymer with reactive monomer groups which facilitate fusion bonding to the catheter part.
7. The catheter of claim 6 wherein the reactive monomer groups include at least one component selected from the group consisting of carboxylic acid, acrylic acid and anhydrides thereof.
8. The catheter of claim 1 wherein the inner layer of the tubular member is thicker than the outer layer.
9. The catheter of claim 1 wherein the catheter part bonded to the outer layer is formed of a material selected from the group consisting of polyolefin, polyester, polyamide and copolymers thereof.
10. An intraluminal catheter, comprising:

a) an elongated catheter shaft having proximal and distal ends, a port in the distal end and a lumen extending therein;

b) a first catheter part having a first polymer layer with a desired melting point and a second polymer layer with a melting point greater than the melting point of the first polymer layer; and

c) a second catheter part fusion bonded to the first polymer layer of the first catheter part.

11. The catheter of claim 1 wherein the second polymer layer has a static coefficient of friction of less than about 0.35.

12. The catheter of claim 10 wherein the second polymer layer has a static coefficient of friction of less than about 0.30.

13. The catheter of claim 10 wherein the first polymer layer is formed of a polyolefin adhesive polymer.

14. The catheter of claim 13 wherein the polyolefin adhesive polymer is a copolymer formed with up to 30% by weight of reactive monomer groups which facilitate fusion bonding to the second catheter part.

15. The catheter of claim 14 wherein the reactive monomer groups include at least one component selected from the group consisting of carboxylic acid, acrylic acid, and anhydrides thereof.

16. The catheter of claim 10 wherein the second polymer layer of the tubular member is much thicker than the first polymer layer.

17. The catheter of claim 10 wherein the second catheter part is formed of a material selected from the group consisting of polyolefin, polyester, polyamide and copolymers thereof.

18. A balloon dilatation catheter comprising:

a) an elongated shaft having proximal and distal ends, a port in the distal end and a guidewire lumen extending therein to and in fluid communication with the port in the distal end;

b) a multilayered tubular member defining at least in part the guidewire lumen extending to the port in the distal end having an inner layer formed of a lubricious polymeric material and an outer layer formed of a

polymeric material having a melting point less than that of the lubricious polymeric material of the adjacent inner layer; and

c) a catheter part fusion bonded to the outer layer of the inner tubular layer.

5 19. The catheter of claim 18 wherein the catheter part is a distal skirt of a dilatation balloon.

20. The catheter of claim 18 wherein the inner layer has a static coefficient of friction of less than about 0.35.

10 21. The catheter of claim 18 wherein the inner layer has a static coefficient of friction of less than about 0.30.

22. The catheter of claim 18 wherein the outer layer is a polyolefin adhesive polymer.

15 23. The catheter of claim 22 wherein the polyolefin is a copolymer formed with up to 30% by weight of reactive monomer groups which facilitate fusion bonding of the outer layer to the catheter part.

24. The catheter of claim 23 wherein the reactive monomer groups include at least one component selected from the group consisting of carboxylic acid, acrylic acid, maleic acid and anhydrides thereof.

20 25. The catheter of claim 18 wherein the inner layer of the multilayered tubular member is much thicker than the outer layer.

26. The catheter of claim 18 wherein the catheter part is formed of a material selected from the group consisting of polyolefin, polyester, polyamide and copolymers thereof.

27. An intraluminal catheter comprising:

25 a) an elongated shaft having proximal and distal ends, a port in the distal end and a guidewire lumen extending therein to and in fluid communication with the port in the distal end;

30 b) a multilayered tubular member having an inner layer formed of a lubricious polymeric material which defines in part the guidewire lumen and an outer layer formed of a polymeric material having a lower melting point than the melting point of the polymeric material of the inner layer; and

- c) a non-traumatic distal tip on the distal end of the catheter formed by an extension of the outer layer of the multilayered tubular member.

28. The catheter of claim 27 wherein the extension of the outer layer of the multilayered tubular member forms the port in the distal end of the catheter.

5 29. An elongated catheter shaft, comprising:

- a) a catheter wall defining at least in part a lumen extending therein;
- b) an inner layer which defines at least in part the lumen extending within the shaft and which terminates at a location proximal to the distal end of the catheter; and
- c) an outer layer which is more flexible than the inner layer and which extends distally beyond the location where the inner layer terminates, forming a non-traumatic distal end of the catheter shaft.

10 30. The catheter of claim 29 wherein an inner layer is formed of a lubricious polymeric material.

31. The catheter of claim 29 wherein the inner layer has a static coefficient of friction of less than about 0.3.

32. The catheter of claim 29 wherein the inner layer has a static coefficient of friction of less than about 0.30.

20 33. The catheter of claim 29 wherein the inner layer is formed of polymeric material having a desired melting point and the outer layer is formed of a polymeric material having a melting point of at least about 20° C. less than the melting point of the inner layer.

25 34. The catheter of claim 29 wherein the inner layer is formed of polymeric material having a desired melting point and the outer layer is formed of a polymeric material having a melting point of at least about 30° C. less than the melting point of the inner layer.

35. The catheter of claim 29 wherein the outer layer is a polyolefin adhesive polymer.

30 36. The catheter of claim 35 wherein the polyolefin adhesive polymer is a copolymer which has been formed with up to 30% by weight of a monomer with reactive groups which facilitate fusion forming of the distal end of the catheter.

37. The catheter of claim 36 wherein the monomer is selected from the group consisting of carboxylic acid, acrylic acid, maleic acid and anhydrides thereof.

38. The catheter of claim 29 wherein the inner layer is thicker than the outer layer.

5 39. An elongated tubular member, comprising:

a) a tubular wall having a lumen extending therein;

b) an inner layer of the tubular wall which defines at least in part the lumen extending therein and which is formed of lubricious polymeric material having a desired melting point; and

10 c) an outer layer of the tubular wall which is more flexible than the inner layer and which has a melting point at least 20° C. less than the melting point of the inner layer.

40. The tubular member of claim 39 wherein the inner layer has a static coefficient of friction of less than about 0.35.

15 41. The tubular member of claim 40 wherein the inner layer has a static coefficient of friction of less than about 0.30.

42. The tubular member of claim 39 wherein the outer layer is a polyolefin adhesive polymer.

20 43. The tubular member of claim 42 wherein the polyolefin adhesive polymer is copolymer formed of up to 30% by weight of a monomer with reactive groups which facilitate fusion forming of the distal end of the catheter.

44. The catheter of claim 42 wherein the monomer is selected from the group consisting of carboxylic acid, acrylic acid, maleic acid and anhydrides thereof.

25 45. An intraluminal catheter part comprising an elongated multilayered tubular member having an inner lubricious layer and an adjacent polymeric layer having a melting point of at least 20° C. less than the inner layer.

46. The intraluminal catheter part of claim 45 wherein the polymeric layer adjacent the inner lubricious layer has a melting point of at least about 30° C. less than the inner layer.

30 47. The intraluminal catheter part of claim 44 wherein the adjacent polymeric layer is formed of a polyolefin copolymerized with one or more

components selected from the group consisting of carboxylic acid, acrylic acid and an anhydrides thereof.

48. The intraluminal catheter part of claim 45 wherein the component with which the polyolefin is copolymerized is unsaturated.

5 49. An intraluminal catheter comprising:

a) an elongated shaft having proximal and distal ends, a port in the distal end and a guidewire lumen extending therein to and in fluid communication with the port in the distal end;

10 b) a multilayered tubular member having an inner layer formed of a lubricious polymeric material which defines in part the guidewire lumen and an outer layer formed of a polymeric material having a lower melting point than the melting point of the polymeric material of the inner layer; and

15 c) a non-traumatic distal tip on the distal end of the catheter formed by a tubular member formed of flexible polymeric material which is secured to the outer layer of the multilayered tubular member or the distal end thereof.

50. The catheter of claim 49 wherein the distal tip is secured to the outer layer of the multilayered tubular member by fusion bonding.

20 51. The catheter of claim 48 wherein the non-traumatic distal tip has an outer layer and an inner layer, with the inner layer formed of low melting point polymeric material to facilitate fusion bonding to the outer layer of the multilayered tubular member.

25 52. The catheter of claim 48 wherein the outer layer of the multilayered tubular member has a melting point of at least about 20° C. less than an adjacent polymeric layer.

53. The catheter of claim 48 wherein the outer layer of the multilayered tubular member has a melting point of at least about 30° C. less than an adjacent polymeric layer.

1/2

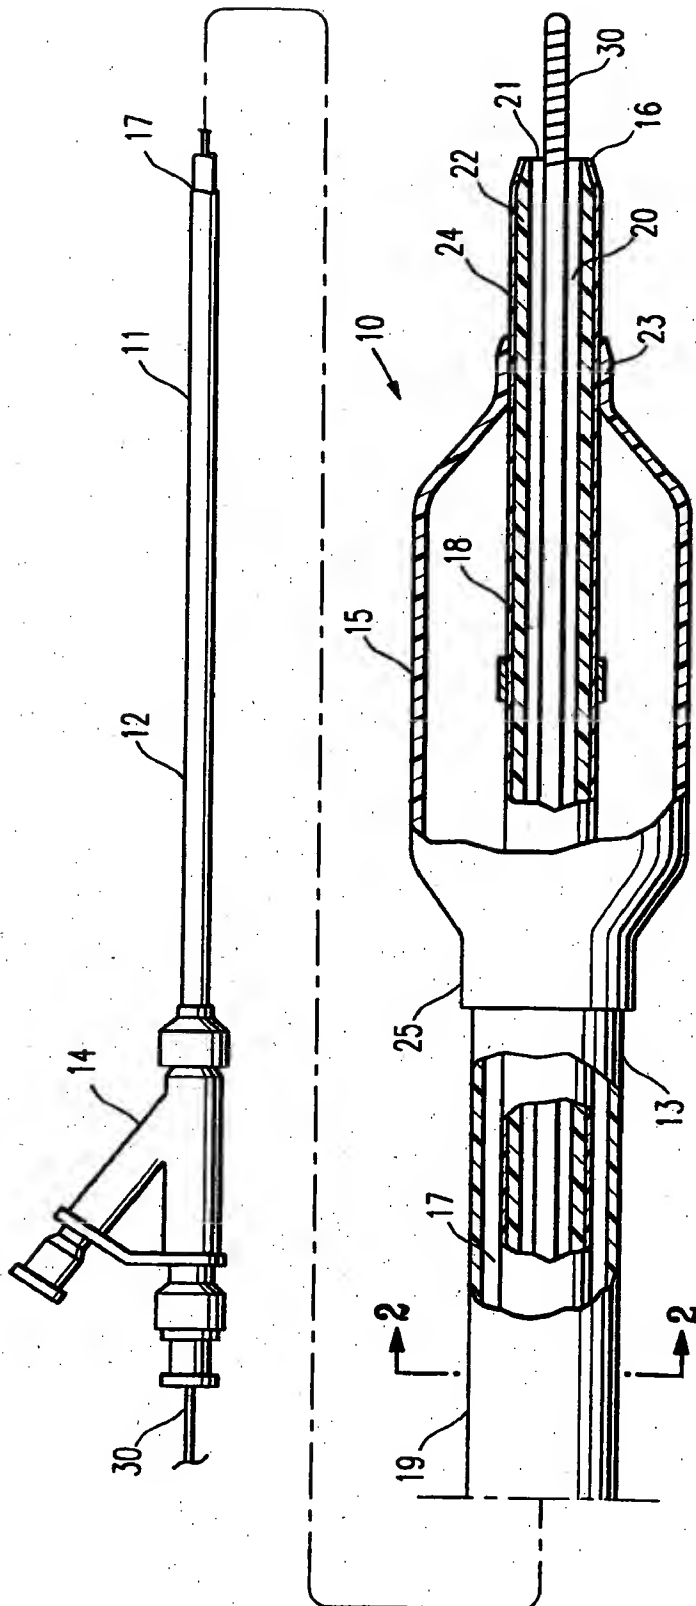


FIG. 1

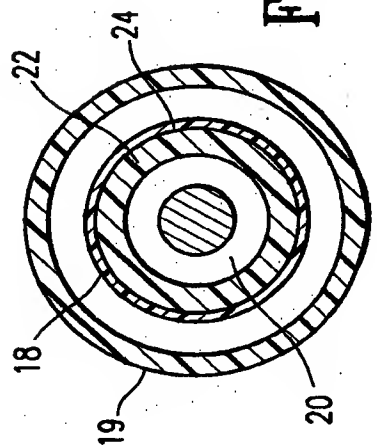


FIG. 2

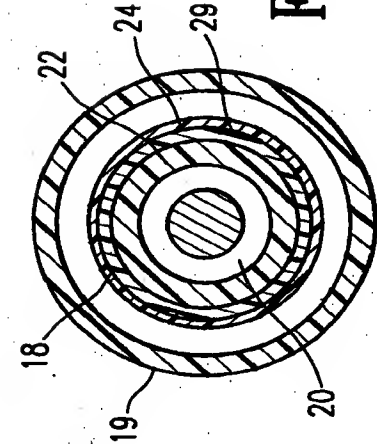


FIG. 4

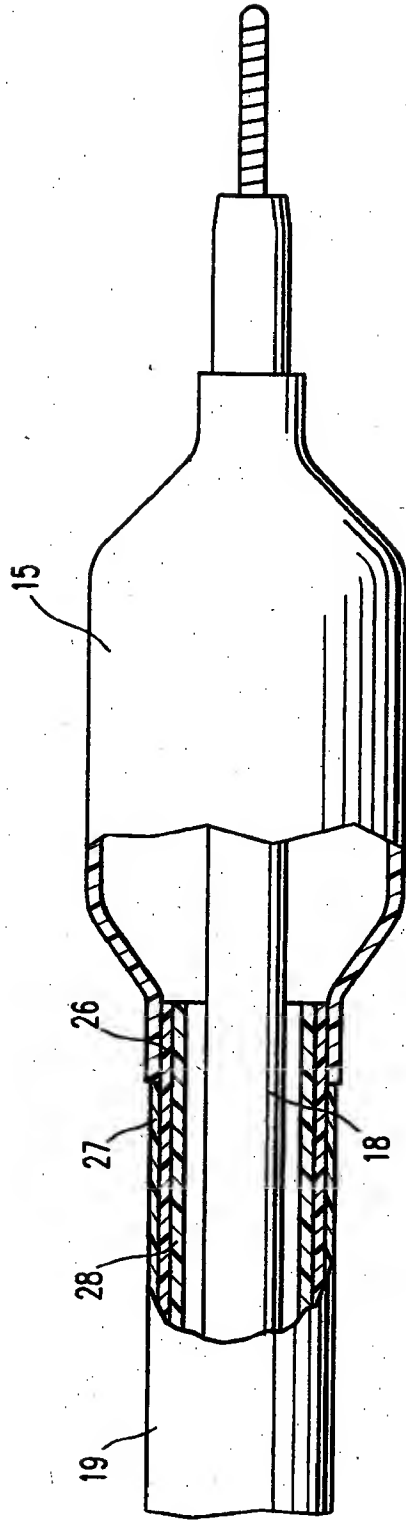


FIG. 3

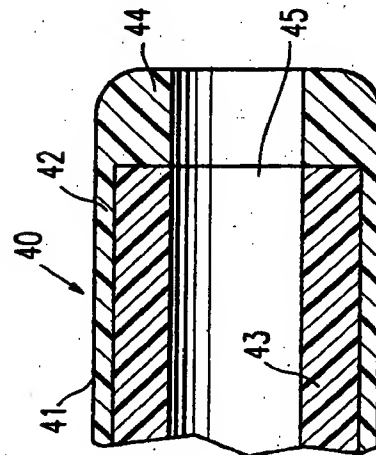


FIG. 5

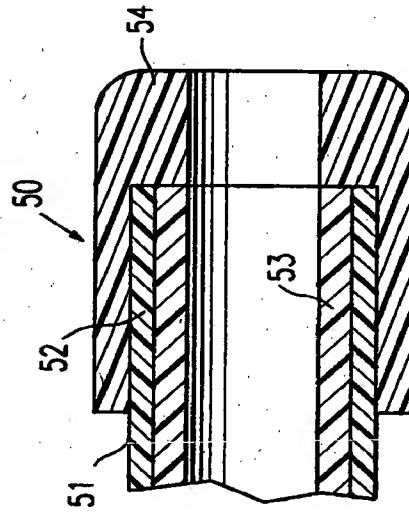


FIG. 6

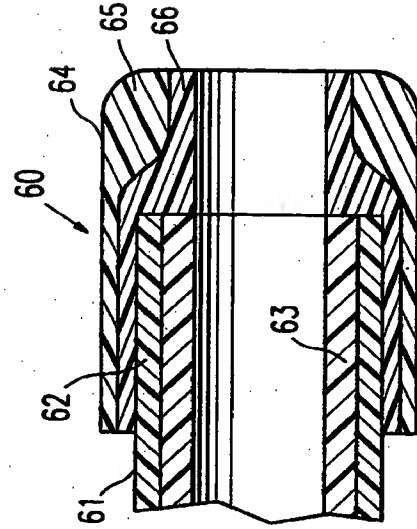


FIG. 7

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 98/24927

A. CLASSIFICATION OF SUBJECT MATTER
IPC 6 A61M25/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 6 A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X A	EP 0 807 446 A (CORDIS) 19 November 1997 see column 3, line 35 - column 5, line 18; figures	27-30, 35 1, 5, 10, 13, 18, 22, 39, 42, 45, 47, 49
X A	US 5 669 920 A (CONLEY) 23 September 1997 see column 10, line 30 - column 11, line 15; figures	39-41, 45, 46 1, 3, 4, 10-12, 18, 20, 21, 27, 29, 31-34, 49, 52, 53
	--- -/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"A" document member of the same patent family

Date of the actual completion of the international search

1 April 1999

Date of mailing of the international search report

12/04/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Kousouretas, I

INTERNATIONAL SEARCH REPORT

Int. l. Application No.

PCT/US 98/24927

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 270 086 A (HAMLIN) 14 December 1993 see column 5, line 8 - line 24; figures ---	1,2,5, 10,13, 18,19,22
A	EP 0 745 395 A (ETHICON) 4 December 1996 see column 7, line 4 - line 17; figures ---	1,10,18
A	US 5 545 149 A (BRIN) 13 August 1996 see claim 1; figures ---	49,50
A	EP 0 334 640 A (BAXTER) 27 September 1989 see abstract; figures ---	49,50
A	US 4 690 175 A (OUCHI) 1 September 1987 see abstract; figures ---	1,10,18, 49
P,X	WO 97 44082 A (PERCUSURGE) 27 November 1997	1,10,18
A	see page 5, line 27 - page 6, line 25; figures -----	39,45,49

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 98/24927

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 807446	A	19-11-1997	US 5851464 A CA 2204808 A JP 10066726 A	22-12-1998 13-11-1997 10-03-1998
US 5669920	A	23-09-1997	US 5527325 A	18-06-1996
US 5270086	A	14-12-1993	AT 91638 T AU 626103 B AU 6317290 A CA 2025962 A,C DE 69002295 T DK 420488 T EP 0420488 A ES 2043289 T IE 64203 B JP 10043287 A JP 3205064 A NO 178424 B	15-08-1993 23-07-1992 28-03-1991 26-03-1991 04-11-1993 30-08-1993 03-04-1991 16-12-1993 12-07-1995 17-02-1998 06-09-1991 18-12-1995
EP 745395	A	04-12-1996	US 5833657 A AU 5246696 A CA 2177528 A JP 9099087 A	10-11-1998 12-12-1996 01-12-1996 15-04-1998
US 5545149	A	13-08-1996	AU 2289795 A DE 69503623 D EP 0758259 A JP 9505507 T WO 9529726 A	29-11-1995 27-08-1998 19-02-1997 03-06-1997 09-11-1995
EP 334640	A	27-09-1989	US 5078702 A JP 1310666 A	07-01-1992 14-12-1989
US 4690175	A	01-09-1987	JP 1746158 C JP 3029406 B JP 58086129 A DE 3242449 A US 4899787 A US 4495134 A	25-03-1993 24-04-1991 23-05-1983 26-05-1983 13-02-1990 22-01-1985
WO 9744082	A	27-11-1997	AU 3071797 A AU 3071897 A AU 3132097 A CA 2255684 A EP 0904125 A EP 0901392 A WO 9744084 A WO 9744085 A US 5868705 A US 5833644 A	09-12-1997 09-12-1997 09-12-1997 27-11-1997 31-03-1999 17-03-1999 27-11-1997 27-11-1997 09-02-1999 10-11-1998

THIS PAGE BLANK (USPTO)